

東業德勤測試顧問有限公司  
ETS-TESTCONSULT LIMITED

8/F., Block B, Veristrong Industrial Centre, 34-36 Au Pui Wan Street, Fotan, Hong Kong  
Tel : 2695 8318 E-mail : etl@ets-testconsult.com  
Fax : 2695 3944 Web site : www.ets-testconsult.com


**TEST REPORT**

**Internal Calibration Report**  
of  
**Dust Trak Monitor**

**Manufacturer** : TSI - 8520 Dust Trak      **Date of Calibration** : 14 July 2008  
**Serial No.** : 15115 (ET/EA/001/02)      **Calibration Due Date** : 13 January 2009  
**Method** : Parallel measurement (five-point calibration) by placing the Dust Trak Monitor and High Volume Air Samper together under the same environmental condition

**Results** :


Dust Trak Monitor (ug/m <sup>3</sup> )	36	50	72	154	221
High Volume Air Sampler (ug/m <sup>3</sup> )	32	42	62	140	181
Serail No of High Volume Air Sampler : 1178			Calibration Date: 01 September 2008		

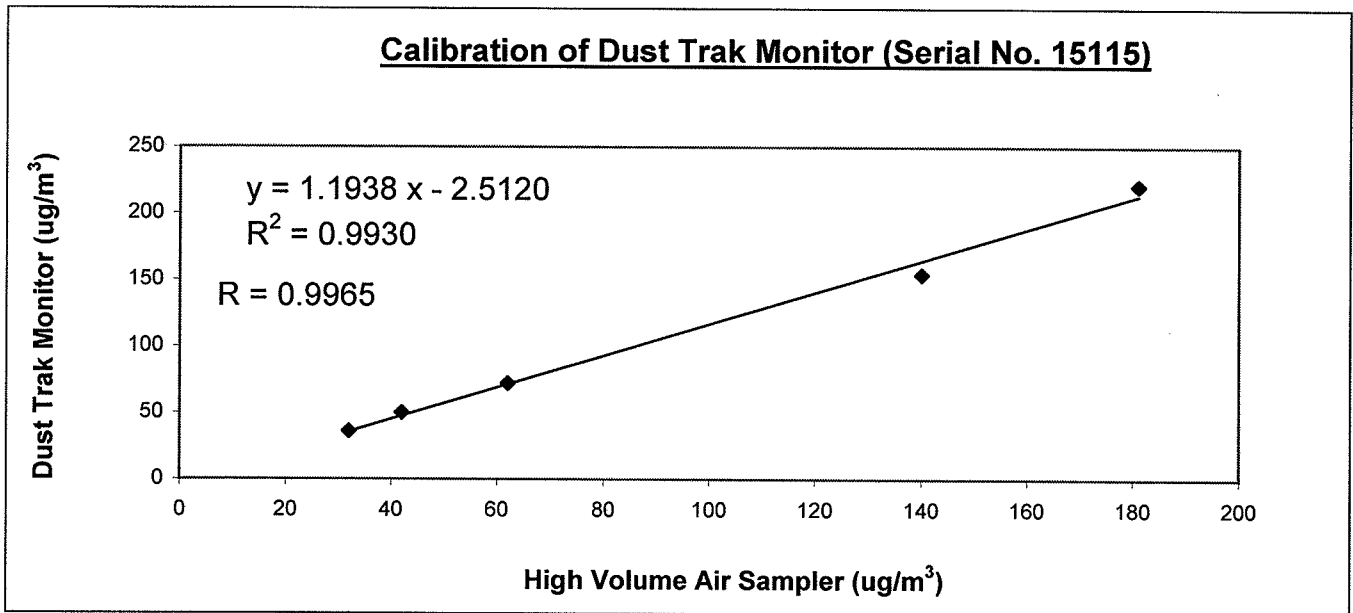



Acceptance Criteria :

Correlation coefficient (r) of the calibration curve greater than 0.990 after a five point calibration

The Dust Trak Monitor complies \* / does not comply \* with the internal calibration procedures and is deemed acceptable \* / unacceptable \* for use.

Calibrated by :   
LEUNG, Ka Ming  
(Assistant Environmental Officer)

Approved by :   
LAW, Sau Yee  
(Senior Environmental Officer)



東業德勤測試顧問有限公司  
ETS-TESTCONSULT LIMITED

8/F., Block B, Veristrong Industrial Centre, 34-36 Au Pui Wan Street, Fotan, Hong Kong  
Tel : 2695 8318 E-mail : etl@ets-testconsult.com  
Fax : 2695 3944 Web site : www.ets-testconsult.com

**TEST REPORT**


**Calibration Report**  
of  
**High Volume Air Sampler**

**Manufacturer** : Graseby GMW      **Date of Calibration** : 05 September 2008  
**Serial No.** : 9035 (ET / EA / 003 / 09)      **Calibration Due Date** : 04 November 2008  
**Method** : Based on Operations Manual for in series calibration method by TISCH  
ENVIROMENTAL Model Te-5025A calibration kit

**Results** :

Flow recorder reading (cfm)	53	47	42	32	25
Qstd (Actual flow rate, m <sup>3</sup> /min)	1.57	1.39	1.24	0.99	0.78
Pressure :	760.56 mm Hg		Temp. :	299 K	

**Sampler 9035 Calibration Curve**  
**Site: Kwai Chung I P (L-1)**  
**Date of Calibration: 05 September 2008**

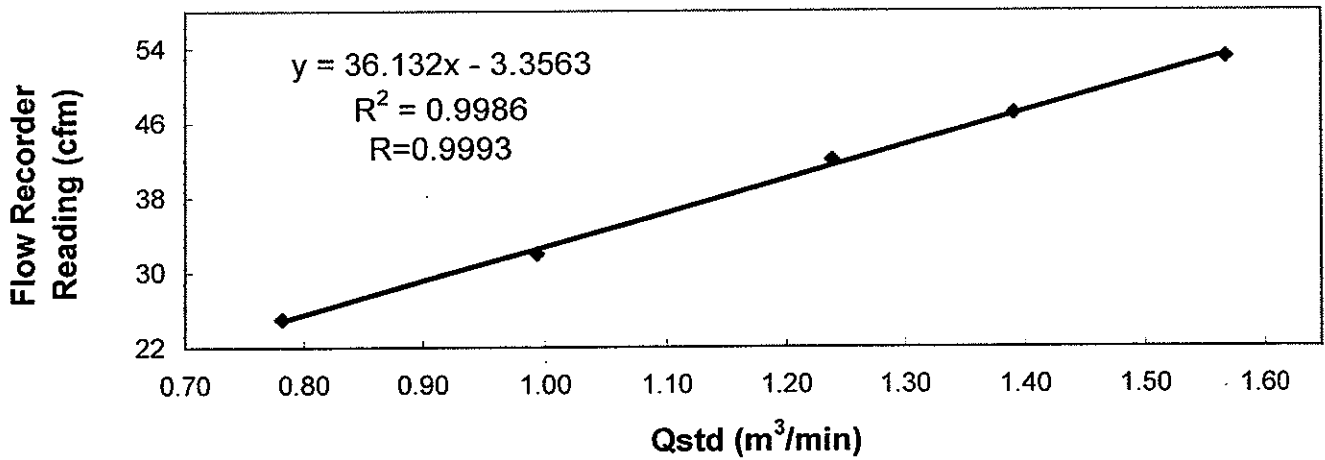

Acceptance Criteria : Correlation coefficient (r) of the calibration curve greater than 0.990 after a 5-point calibration

The high volume sampler complies \* / does not comply \* with the specified requirements and is deemed acceptable \* / unacceptable \* for use.

Calibrated by : MAK, Kei Wai  
MAK, Kei Wai  
(Senior Technician)

Approved by : CHOW, Hoi Tat  
CHOW, Hoi Tat  
(Assistant Environmental Officer)