

Hip Hing Joint Venture

Hong Kong Convention and
Exhibition Centre Expansion
Project: *6th and Final Operational
Phase Monthly Environmental
Monitoring and Audit Report*

January 2011

Environmental Resources Management

21/F Lincoln House
979 King's Road
Taikoo Place
Island East, Hong Kong
Telephone: (852) 2271 3000
Facsimile: (852) 2723 5660
E-mail: post.hk@erm.com
<http://www.erm.com>

Hip Hing Joint Venture

Hong Kong Convention and
Exhibition Centre Expansion
Project: *6th and Final Operational
Phase Monthly Environmental
Monitoring and Audit Report*

January 2011

Reference 0050690

For and on behalf of ERM-Hong Kong, Limited	
Approved by:	<u>Dr. Robin Kennish</u>
Signed:	<u></u>
Position:	<u>Director</u>
Certified by:	<u></u>
(Environmental Team Leader - Winnie Ko)	
Date:	<u>26 January 2011</u>

This report has been prepared by ERM Hong-Kong, Limited with all reasonable skill, care and diligence within the terms of the Contract with the client, incorporating our General Terms and Conditions of Business and taking account of the resources devoted to it by agreement with the client.

We disclaim any responsibility to the client and others in respect of any matters outside the scope of the above.

This report is confidential to the client and we accept no responsibility of whatsoever nature to third parties to whom this report, or any part thereof, is made known. Any such party relies on the report at their own risk.



NATURE & TECHNOLOGIES (HK) LIMITED
科技環保(香港)有限公司

Unit 908, 9/F., Elite Industrial Centre, 883 Cheung Sha Wan Road, Cheung Sha Wan, Kowloon
九龍長沙灣長沙灣道883號億利工業中心9樓908室 Tel 電話 : (852) 2877 3122 Fax 傳真 : (852) 2511 0922
Email 電郵 : enquiry@nt.com.hk Web page 網址 : http://www.nt.com.hk

Our Ref: 3.16/014/2006/gl

26 January 2011

Maunsell Consultants Asia Ltd
Grand Central Plaza, Tower 2
138 Shatin Rural Committee Road
Shatin, N.T., Hong Kong

Attn: Ms Marian Kwok
Senior Project Manager

Dear Ms Kwok,

**Hong Kong Convention and Exhibition Centre Expansion Project:
6th and Final Operational Phase Monthly Environmental Monitoring and Audit Report
(Environmental Permit No. EP-239/2006/B)**

With reference to the captioned document concerning the operational phase EM&A received from the ET on 25 January 2011, we are pleased to provide our verification for the document pursuant to condition 3 of the Environmental Permit (EP) No. EP-239/2006/B.

Yours faithfully,
Nature & Technologies (HK) Limited

Ir Dr Gabriel C K Lam
Director

- cc: - Hong Kong Trade Development Council (Attn: Mr. K. F. Chan)
- Hip Hing Ngo Kee Joint Venture (Attn: Mr. Eric Lau & Mr. William Tam)
- ERM (Attn: Ms. Winnie Ko)

CONTENTS

	<i>EXECUTIVE SUMMARY</i>	<i>I</i>
<i>1</i>	<i>INTRODUCTION</i>	<i>1</i>
<i>1.1</i>	<i>PURPOSE OF THE REPORT</i>	<i>1</i>
<i>1.2</i>	<i>STRUCTURE OF THE REPORT</i>	<i>1</i>
<i>2</i>	<i>PROJECT INFORMATION</i>	<i>3</i>
<i>2.1</i>	<i>BACKGROUND</i>	<i>3</i>
<i>2.2</i>	<i>LOCATION OF PROJECT</i>	<i>4</i>
<i>2.3</i>	<i>PROJECT ORGANISATION</i>	<i>4</i>
<i>2.4</i>	<i>STATUS OF ENVIRONMENTAL APPROVAL DOCUMENTS</i>	<i>4</i>
<i>3</i>	<i>ENVIRONMENTAL MONITORING METHODOLOGY</i>	<i>5</i>
<i>3.1</i>	<i>AIR QUALITY MONITORING</i>	<i>5</i>
<i>4</i>	<i>IMPLEMENTATION STATUS ON ENVIRONMENTAL PROTECTION REQUIREMENTS</i>	<i>9</i>
<i>5</i>	<i>MONITORING RESULTS</i>	<i>10</i>
<i>6</i>	<i>ENVIRONMENTAL NON-CONFORMANCE</i>	<i>11</i>
<i>7</i>	<i>FUTURE KEY ISSUES</i>	<i>12</i>
<i>7.1</i>	<i>KEY ISSUES FOR THE COMING MONTH</i>	<i>12</i>
<i>7.2</i>	<i>MONITORING SCHEDULE FOR THE COMING MONTHS</i>	<i>12</i>
<i>8</i>	<i>REVIEW OF THE EM&A DATA AND EIA PREDICTIONS</i>	<i>13</i>
<i>8.1</i>	<i>AIR QUALITY</i>	<i>13</i>
<i>8.2</i>	<i>CONCLUSION OF REVIEW</i>	<i>14</i>
<i>9</i>	<i>CONCLUSIONS</i>	<i>15</i>

LIST OF TABLES

Table 2.1	Summary of Environmental Licensing, Notification and Permit Status
Table 3.1	Air Monitoring Stations
Table 3.2	TSP Monitoring Parameter and Frequency
Table 3.3	Action and Limit Levels for NO ₂
Table 3.4	NO ₂ Monitoring Equipment
Table 8.1	Comparison of NO ₂ Concentration predicted in the EIA, Tunnel Air Quality Guidelines and the Air Quality Monitoring Results

LIST OF ANNEXES

Annex A	Location of Project
Annex B	Project Organization Chart and Contact Detail
Annex C	Location of NO ₂ Quality Monitoring Station
Annex D	Monitoring Schedule for the Reporting Period and the Following Month
Annex E	Calibration Certificates for NO ₂ Analyzer, Flow Meter, Mass-flow Controllers and Certificates for Calibration Gas
Annex F	Event / Action Plans for Air Quality Monitoring
Annex G	NO ₂ Monitoring Results

EXECUTIVE SUMMARY

The operational phase air quality monitoring for Hong Kong Convention and Exhibition Centre Expansion Project (EIAO Register No: AEIAR-100/2006) commenced on 6 July 2010. This is the sixth and final Environmental Monitoring and Audit (EM&A) report presenting the EM&A data carried out during the period from 1 December 2010 to 10 January 2011 in accordance with the EM&A Manual. One-hour NO₂ monitoring was carried out continuously at the designated monitoring station (AM3) under the Atrium Link Extension during this reporting period. This monitoring commenced on 6 July 2010 for a total of six months.

This report summarises and analyses the air quality monitoring data collected in the reporting period (1 December 2010 to 10 January 2011) as well as those collected over the six-month monitoring period (6 July 2010 to 10 January 2011).

No exceedance of the Action and Limit Levels of 1-hour NO₂ was recorded at the designated monitoring station under the ALE in this reporting period.

Over the six-month monitoring period, only one exceedance of the Action and Limit Level of 1-hour NO₂ was recorded on 8 September 2010 as a result of heavy and stalled traffic under the Project due to opening of the Horse Race Meeting in Happy Valley. The NO₂ monitoring data from the six-month monitoring period confirmed that no adverse impact environmental impact would be initiated from the operation of the Project. Exceedance of hourly NO₂ AQO criteria was observed to be transient and occasional, and relocation of fresh air intakes implemented during the design stage has also mitigated the impacts to nearby sensitive receivers.

The six-month monitoring program of hourly NO₂ concentration under the Project has been completed at the end of this reporting month, and therefore

NO₂ monitoring was terminated on 11 January 2011.

ERM-Hong Kong, Limited (ERM) was appointed by Hip Hing Joint Venture as the Environmental Team (ET) for the operational phase Environmental Monitoring and Audit (EM&A) programme for Hong Kong Convention and Exhibition Centre Expansion Project (the Project).

1.1 PURPOSE OF THE REPORT

This is the sixth and final EM&A report for the operational phase. It summarises the results for air quality monitoring conducted under the Atrium Link Extension (ALE) of the Hong Kong Convention and Exhibition Centre (HKCEC) for the period of 1 December 2010 to 10 January 2011. It also summarises and analyses the air quality monitoring data collected over the six-month monitoring period from 6 July 2010.

1.2 STRUCTURE OF THE REPORT

The structure of the report is as follows:

Section 1 : **Introduction**

details the scope and structure of the report;

Section 2 : **Project Information**

summarises background and scope of the Project, project organisation and contact details during the reporting period and the six-month monitoring period;

Section 3 : **Environmental Monitoring Requirement**

summarises the monitoring parameters, monitoring programmes, monitoring methodologies, monitoring frequency, monitoring locations, Action and Limit Levels and Event / Action Plans;

Section 4 : **Implementation Status on Environmental Mitigation Measures**

summarises the implementation of environmental protection measures during the reporting period and the six-month monitoring period;

Section 5 : **Monitoring Results**

summarises the monitoring results obtained in the reporting period and the six-month monitoring period;

Section 6 : **Environmental Non-conformance**

summarises any environmental exceedance, environmental complaints and environmental summons received within the reporting period and the six-month monitoring period;

Section 7: **Future Key Issues**

summarises the impact forecast and monitoring schedule for the next month;

Section 8: **Review of EM&A Data and EIA Predictions**

compares and contrasts the EM&A data in the reporting period and the six-month monitoring period with the EIA predictions and annotates with explanation for any discrepancies; and,

Section 9: **Conclusion**

2.1

BACKGROUND

The Hong Kong Trade Development Council (HKTDC) expanded its existing facilities to provide additional space for Hong Kong's leading trade fairs to be held at the HKCEC. The Project is located in North Wan Chai and occupies the aerial space between Phase I and Phase II of the HKCEC. The new ALE spans across the water channel between Phase I and Phase II of the HKCEC to accommodate three main levels of Exhibition Hall Extensions. The level of the main roof of the Extension is similar in height to the podium roof of the Phase I building. A northern row of permanent supporting columns are located on land close to Expo Drive Central and similarly a southern row of columns land near to Convention Avenue. There are no permanent intermediate columns in the waterway.

The potential environmental impacts of the Project have been studied in the "Hong Kong Convention and Exhibition Centre, Atrium Link Extension – Environmental Impact Assessment Report" (EIAO Register No: AEIAR-100/2006) (the EIA Report). The EIA Report was approved on 21 April 2006 under the *Environmental Impact Assessment Ordinance* (EIAO). An Environmental Permit (EP-239/2006) for the works was granted on 12 May 2006. An application for variation of the Environmental Permit was made on 25 January 2007, an amended Environmental Permit (EP-239/2006/A) was granted on 12 February 2007. An application for further variation of the Environmental Permit was made on 18 April 2008, and an amended Environmental Permit (EP-239/2006/B) was granted on 12 May 2008. Under the requirements of Condition 3.1 of Environmental Permit EP-239/2006/B, an EM&A programme as set out in the EM&A Manual and its supplement is required to be implemented.

The EIA Study for the Project considered that vehicular exhaust emissions from the road traffic under the ALE may pose an air quality concern with the more confined conditions created by the ALE. Post-construction/operational phase monitoring of nitrogen dioxide (NO₂) under the ALE for six months was recommended.

All construction works at the ALE were completed in October 2009. A proposal for the NO₂ monitoring location (the Proposal) was submitted to Environmental Protection Department (EPD) on 18 November 2009 (*HHJV Letter Ref No. AKWL:VCML:nlwy: 98705/EN100-797*), which was approved via EPD's Letter Ref No. (3) in EP2/H5/A/14/Pt.11 on 11 December 2009. Owing to various technical issues encountered during the testing and commissioning of monitoring equipment, the NO₂ monitoring programme was only formally started on 6 July 2010. NO₂ monitoring was required to be conducted for at least six months. The six-month monitoring of hourly NO₂ was completed at the end of reporting period and was terminated on 11 January 2011.

The second multi-point calibration check with mass flow controllers was completed on 31 December 2010. The monitoring data presented in the reporting month were adjusted with reference to the respective check results accordingly. Monitoring results collected in between 6 July and 30 November 2010 were adjusted with reference to the check results conducted on 29 October 2010.

2.2 LOCATION OF PROJECT

The location of the Project is shown in *Annex A*.

2.3 PROJECT ORGANISATION

The Project organization chart and contact details are shown in *Annex B*.

2.4 STATUS OF ENVIRONMENTAL APPROVAL DOCUMENTS

A summary of the relevant permits, licences, and/or notifications on environmental protection for this Project since August 2006 is presented in *Table 2.1*.

Table 2.1 *Summary of Environmental Licensing, Notification and Permit Status*

Permit/ Licenses/ Notification	Reference	Validity Period	Remarks
Environmental Permit	EP-239/2006/B	Throughout the Contract	Environmental Permit (EP) EP-239/2006 granted originally on 12 May 2006. Since then the EP have been varied twice. The latest revised EP was issued on 12 May 2008
Proposal for Termination of Construction Phase EM&A Programme	-	-	Approved on 4 November 2009 by EPD.
Proposal for NO ₂ Monitoring Location during Initial Operational Phase	-	-	Approved on 11 December 2009 by EPD.

3.1 AIR QUALITY MONITORING

3.1.1 Monitoring Location

In accordance with the EM&A Manual, monitoring of NO₂ levels was conducted at the monitoring station described in *Table 3.1*. A map and a photograph showing the monitoring station are presented in *Annex C*. *Figure C1* in *Annex C* has been updated from the version provided in the Proposal as the revised figure indicates the correct proposed location for the NO₂ monitoring equipment setup.

Table 3.1 *Air Monitoring Stations*

Monitoring Station	Description
AM3	A location immediately north of Convention Avenue under the Atrium Link Extension

3.1.2 Monitoring Parameters, Frequency and Programme

Air quality monitoring was conducted in accordance with the requirements stipulated in the EM&A Manual (*Table 3.2*). The monitoring and equipment checking schedules for the reporting month and the upcoming month are shown in *Annex D*.

Table 3.2 *TSP Monitoring Parameter and Frequency*

Parameter	Frequency
1-hour NO ₂ monitoring	Continuous

3.1.3 Action and Limit Levels

The Action and Limit levels in the EM&A Manual were adopted and these are presented in *Table 3.3*.

Table 3.3 *Action and Limit Levels for NO₂*

Parameter	Air Monitoring Station	Action Level, µgm ⁻³	Limit Level, µgm ⁻³
1-hour NO ₂ monitoring	AM3	300	300

3.1.4 Monitoring Equipment

Continuous monitoring of 1-hour NO₂ levels was performed at the designated monitoring station using an automatic chemiluminescence NO/NO₂/NO_x analyzer with appropriate sampling inlets installed. The performance specification of the analyzer complies with the USEPA reference method in *US EPA Standard Title 40, Code of Federation Regulations Part 53 (USEPA ST 40 CFR 53)*. The sampling flow rate of the analyzer was checked with a portable flow

meter weekly. *Table 3.4* summarises the details of the equipment used for the monitoring.

Table 3.4 *NO₂ Monitoring Equipment*

Monitoring Station	Equipment	Model No.
AM3 (continuous 1-hr NO ₂)	Chemiluminescence NO/NO ₂ /NO _x Analyzer	Teledyne Instruments Model 200E
	DryCal Flow Meter	BIOS International DCL-M
	Mass-flow Controllers	Cole Parmer Instrument Model 56089 and 56090

3.1.5 *Monitoring Methodology*

Installation

The monitoring equipment was placed at a location underneath the ALE as presented in *Annex C*. The monitoring location was chosen so that:

- the monitoring equipment was clear from access to pump rooms, thereby minimizing obstruction to pump room maintenance operations; and
- the selected location was sufficiently close to the key source of emissions (NO₂ emission from road traffic) for obtaining representative monitoring data.

The overall setup of the monitoring station is as follows:

- The analyzer was placed in a lockable wooden enclosure to prevent tampering of the monitoring equipment;
- The air sampling inlet was mounted at a height of 2m above ground with a 1m minimum separation between the tip of the inlet and the side wall so that the air flow is free from physical obstruction;
- The air inlet was connected to the analyzer through a 1/4" teflon tubing with 47mm in-line particulate filter;
- An in-series external pump was provided for drawing in air; and,
- An air-conditioner is installed for the wooden enclosure to maintain the optimal temperature (<32°C) for the operation of the analyzer.

Field Monitoring

- NO, NO_x and NO₂ concentrations (5-min average concentrations) were calculated and logged automatically at 5-minute intervals on a continuous basis;
- The logged data were downloaded on a weekly basis for further analyses; and

- In the event of a zero drift beyond ± 15 ppb and/or a span drift beyond $\pm 15\%$, the data obtained before and after the particular zero/span check would be flagged and excluded from the calculation of the reported 1-hour NO_2 averages. The analyzer will subsequently be re-calibrated as soon as the extraordinary data drift is identified.

3.1.6 *Maintenance and Calibration*

The analyzer and its associated accessories were maintained in good working condition. The operating temperature of the equipment set was maintained below 32°C with an exhaust fan and an air-conditioner. The in-line particulate filter was also replaced bi-weekly to avoid blockage of the air inlet.

The flow rate of the analyzer was verified on a weekly basis by a portable flow meter. Zero check was performed automatically by the analyzer at 00:00 hours each day for 15 to 20 minutes, and three 5-minute average “zero” readings will be measured to validate the “zero” reading recorded by the analyzer.

Span check for NO_2 was also conducted immediately following the zero check with the built-in permeation tube of the analyzer for 15 to 20 minutes, and three 5-minute average “span” readings will also be measured for checking against the drift limits. Manual span checks with standard 400ppb NO gas were conducted on 3, 10, 17, 31 December 2010 and 7 January 2011 to ensure span drift was within the acceptable limits stated in the QA Handbook. The span gas readings were 398, 404, 399, 387 and 398 ppb NO, which fell within the acceptable range of $\pm 15\%$ from 400ppb NO and suggested the monitoring data was valid.

As indicated above, the air flow rate of the analyzer was checked on a weekly basis and maintained at $500 \pm 50 \text{ cm}^3\text{s}^{-1}$ as per specification in the equipment operation manual by the portable flow meter.

Standard nitrogen oxide gases with concentrations of 0 ppb and 400 ppb were used for calibrating the analyzer (2-point calibration) on 10 December 2010 and 7 January 2011. The slopes of the calibration curves were recorded to be 1.05 and 1.09 respectively, complying with the required range of 1.0 ± 0.3 as per required in the operation manual of the analyzer.

The analyzer calibration records, the certificates for calibration gas and the calibration certificate for the portable flow meter are provided in *Annex E*.

A multi-point calibration check was conducted on 31 December 2010 to ensure compliance with requirements in *USEPA ST 40 CFR 53*. The calibration certificates of the mass flow controllers are provided in *Annex E*. The flow rate of gas through the mass-flow controllers were also confirmed using the portable flow meter. NO gas concentrations of 0ppb, 80ppb, 149.8ppb, 200ppb, 300ppb and 400ppb were generated from the standard 0ppb and 400ppb standard NO gas with mass-flow controllers. The gases were then

injected to the analyzer for checking of the accuracy of the calibration curve generated by the 0ppb and 400ppb standard gas. The slope of the multi-point calibration check is 0.988, well within the required range of 1.0 ± 0.3 as per required in the operation manual of the analyzer. The measured span gas concentration in the multi-point check results also fell within the acceptable range of $\pm 15\%$ from standard span NO gas concentrations, suggesting the 2-point calibration practice was valid.

3.1.7 *Event Action Plan*

The Event / Action Plan (EAP) for operational phase air quality monitoring is presented in *Annex F*.

IMPLEMENTATION STATUS ON ENVIRONMENTAL PROTECTION REQUIREMENTS

The environmental concern that led to the requirement for the operational phase EM&A programme is only related to the potential air quality impacts from vehicular exhaust emissions under the ALE. In this regard, the Contractor has relocated the fresh air intakes as per the recommendations of the EIA Report and the relevant EP condition. The other requirement that is relevant in this respect is the six-month NO₂ monitoring under the ALE, which has commenced since 6 July 2010 and is the subject of this report. The six-month monitoring program has been completed and was terminated on 11 January 2011.

Continuous NO₂ monitoring was carried out at the designated monitoring station during the reporting period. The monitoring results for 1-hour NO₂ monitoring corrected with multi-point calibration check results were below both the Action and Limit Levels. The hourly NO₂ concentration was close to 300µgm⁻³ (ie, 299.9 µgm⁻³) in the morning on 21 December 2010, but this high NO₂ concentration was temporary and lasted for no more than 2 hours.

All monitoring data acquired by the analyzer were considered valid as zero/span drift was within the acceptable bounds presented in *Section 3.1.5*. The weekly flow checks confirmed that the sampling flow rate was generally maintained within the acceptable range. The NO₂ monitoring results, a summary of the zero-span check, multi-point calibration check and sampling flow check are provided in *Annex G*. In addition, the monitoring results can also be found at the web-site (<http://www.hkcecema.com/index.html>). The local NO₂ levels near the monitoring station are mainly influenced by vehicular exhaust emissions along Convention Avenue, Expo Drive East and Expo Drive Central.

The NO₂ monitoring results collected over the six-month monitoring period have also been graphically presented together with the results in the reporting period in *Annex G*.

No exceedance of the Action and Limit Levels of 1-hour NO₂ was recorded at the designated monitoring station under the ALE in this reporting period.

Over the six-month monitoring period, only one exceedance of the Action and Limit Level of 1-hour NO₂ was recorded on 8 September 2010.

7 *FUTURE KEY ISSUES*

7.1 *KEY ISSUES FOR THE COMING MONTH*

Emissions from vehicular exhaust on Convention Avenue, Expo Drive Central and Expo Drive East are expected to continue to influence the air quality under the ALE. Since the six-month monitoring period as required in the EM&A Manual of the Project has been completed, NO₂ monitoring was terminated on 11 January 2011.

8.1 AIR QUALITY

During the initial operational phase of the Project, the environmental setting is expected to be similar to those stated in the interim scenario (without WDII and CWB Projects) for quantitative assessment of NO₂ concentration of the approved EIA Report. The monitoring results in the reporting month were compared against the interim NO₂ concentrations predicted in the approved EIA and the criteria for NO₂ concentration in the Air Quality Objective (AQO) and the Tunnel Air Quality Guidelines (TAQG) (Table 8.1).

Table 8.1 Comparison of NO₂ Concentration predicted in the EIA, Tunnel Air Quality Guidelines and the Air Quality Monitoring Results in the Reporting Period

Monitoring Station	Corresponding Location in EIA	NO ₂ concentration in EIA, µgm ⁻³		Air Quality Objective and Tunnel Air Quality Guidelines, µgm ⁻³	Average 1-hour NO ₂ measured from 1 Dec 2010 to 10 Jan 2011, µgm ⁻³	
		Normal Hours	Peak Hours	Standard	Average	Range
AM3	Convention Avenue	146	183	300 ^(a) / 1,800 ^(b)	103.5	17.4 – 299.9

Notes:

(a) 1-hour Air Quality Objective for NO₂

(b) 5-minutes Tunnel Air Quality Criteria in for NO₂.

The monitoring results show that the average hourly NO₂ concentrations recorded are below those predicted in the approved EIA Report, the AQO and the TAQG in the reporting month. The fresh air intakes of Hong Kong Convention and Exhibition Centre Phase I (HKCEC Phase I), Renaissance Harbour View Hotel (Renaissance Hotel) and Grand Hyatt Hotel (Hyatt Hotel) under the ALE have been relocated to the rooftop during the construction phase of the Project as per the requirements in Section 3.61 of the approved EIA Report and Condition 2.9 of EP-239/2006/B. As a result, no adverse air quality impacts are expected on occupants of HKCEC Phase I, Renaissance Hotel and Hyatt Hotel in the reporting month.

The monitoring results in the six-month monitoring period were also compared against the interim NO₂ concentrations predicted in the approved EIA, the AQO and the TAQG (Table 8.2).

Table 8.2 Comparison of NO₂ Concentration predicted in the EIA, AQO, TAQG and the Air Quality Monitoring Results over the Six-month Monitoring Period

Monitoring Station	Corresponding Location in EIA	NO ₂ concentration in EIA, µgm ⁻³		Air Quality Objective and Tunnel Air Quality Guidelines, µgm ⁻³	Average 1-hour NO ₂ measured from 6 July 2010 to 10 January 2011, µgm ⁻³	
		Normal Hours	Peak Hours		Standard	Average
AM3	Convention Avenue	146	183	300 ^(a) / 1,800 ^(b)	82.7	8.1 – 304.2

Notes:

- (a) 1-hour Air Quality Objective for NO₂
- (b) 5-minutes Tunnel Air Quality Criteria in for NO₂.

The monitoring results demonstrated that the average hourly NO₂ levels recorded are below those predicted in the approved EIA Report in the six month monitoring period, the AQO and the TAQG except on 8 September 2010 at 19:00 when the hourly NO₂ concentration was 304.2 µgm⁻³. Investigations revealed that the exceedance might be a result of heavy and extremely slow traffic under the Project due to opening of the Horse Race Meeting in Happy Valley. The exceedance of the hourly NO₂ criteria was only recorded once for an hour over the whole monitoring period and was considered transient.

High NO₂ concentration under the Project was observed to be transient and occasional. The fresh air intakes of HKCEC Phase I, Renaissance Hotel and Hyatt Hotel under the ALE have been relocated to the rooftop during the construction phase of the Project as per the requirements in *Section 3.61* of the approved EIA Report and Condition 2.9 of EP-239/2006/B. As a result, no adverse air quality impacts are expected on occupants of HKCEC Phase I, Renaissance Hotel and Hyatt Hotel during the operation of the Project.

8.2 CONCLUSION OF REVIEW

The EIA predictions and the monitoring results since the commencement of operational monitoring programme have been reviewed. The EIA concluded that the Project would not cause adverse impacts to the environment, and the six-months monitoring results confirmed that environmental impacts from the operation of the Project were transient and occasional. Recommendations given in the EIA are therefore considered to be adequate and effective for minimising the environmental impacts.

The Environmental Monitoring and Audit (EM&A) Report presents the operational phase air quality monitoring conducted during the period from 1 December 2010 to 10 January 2011 in accordance with the EM&A Manual and the requirements under EP-239/2006/B. No exceedance of the Action and Limit Levels of 1-hour NO₂ was recorded at the designated monitoring station under the ALE in this reporting period.

This report also summarises the air quality data collected over the six-month period as required in the EM&A Manual of the Project. A slight exceedance of the Action and Limit Levels of hourly NO₂ was recorded once at the designated monitoring station under the ALE over the six-month period as a result of heavy and stalled traffic under the Project due to opening of the Horse Race Meeting in Happy Valley. As such, it was concluded that no adverse air quality impacts were generated underneath the ALE from operation of the Project. Subsequently, NO₂ monitoring at AM3 was terminated on 11 January 2011 as the six-month NO₂ monitoring as per EM&A requirement was fulfilled at the beginning of the operation phase.

Annex A

Location of Project

Key

 Atrium Link Extension

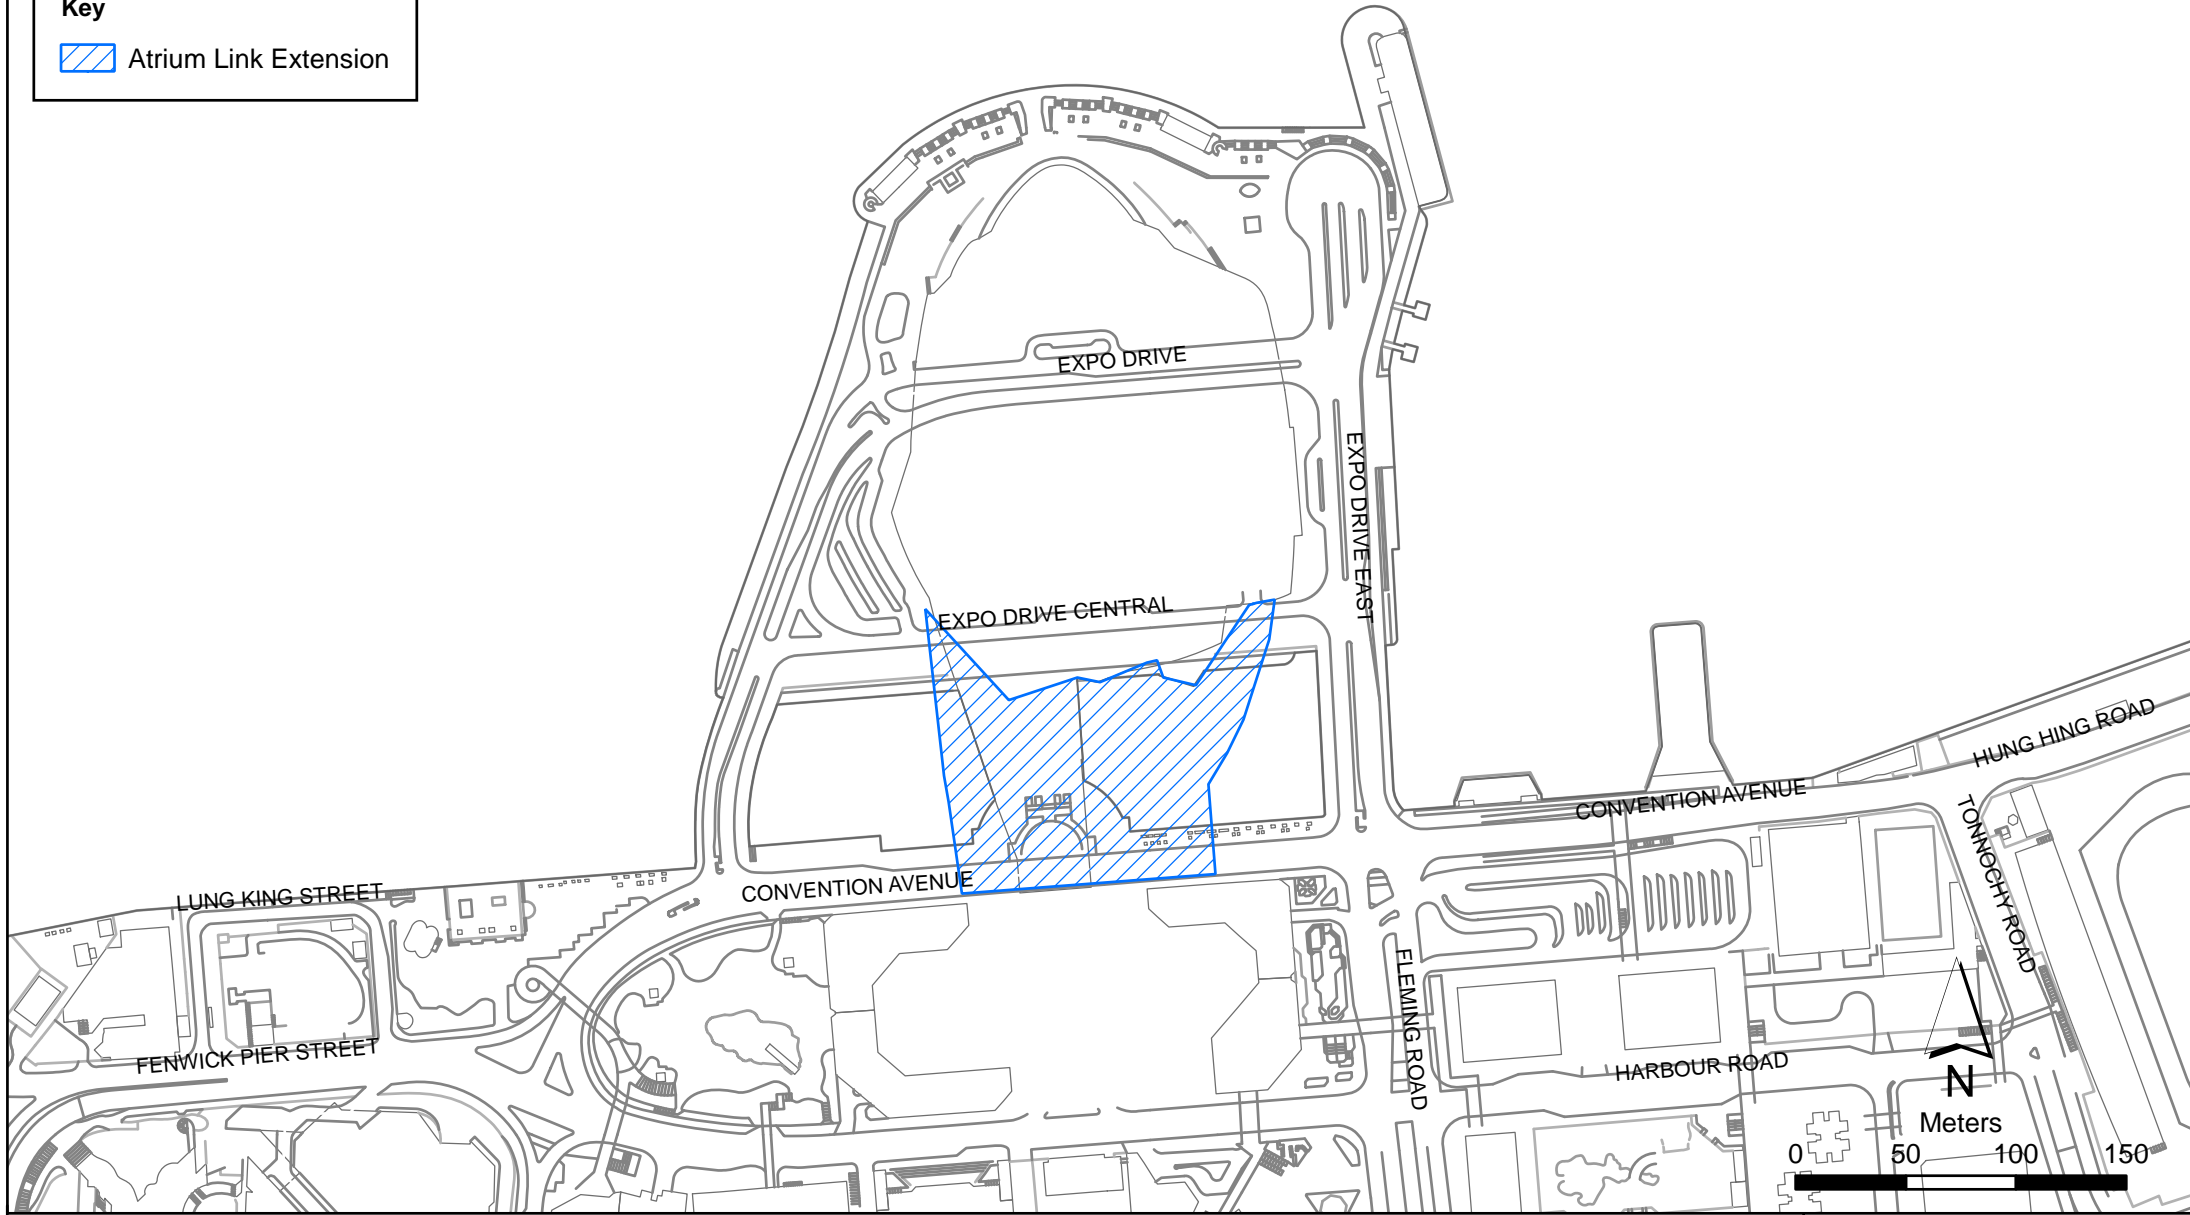



Figure A1

Location of Atrium Link Extension

Annex B

Project Organization Chart and Contact Detail

Project Organization (with contact details)

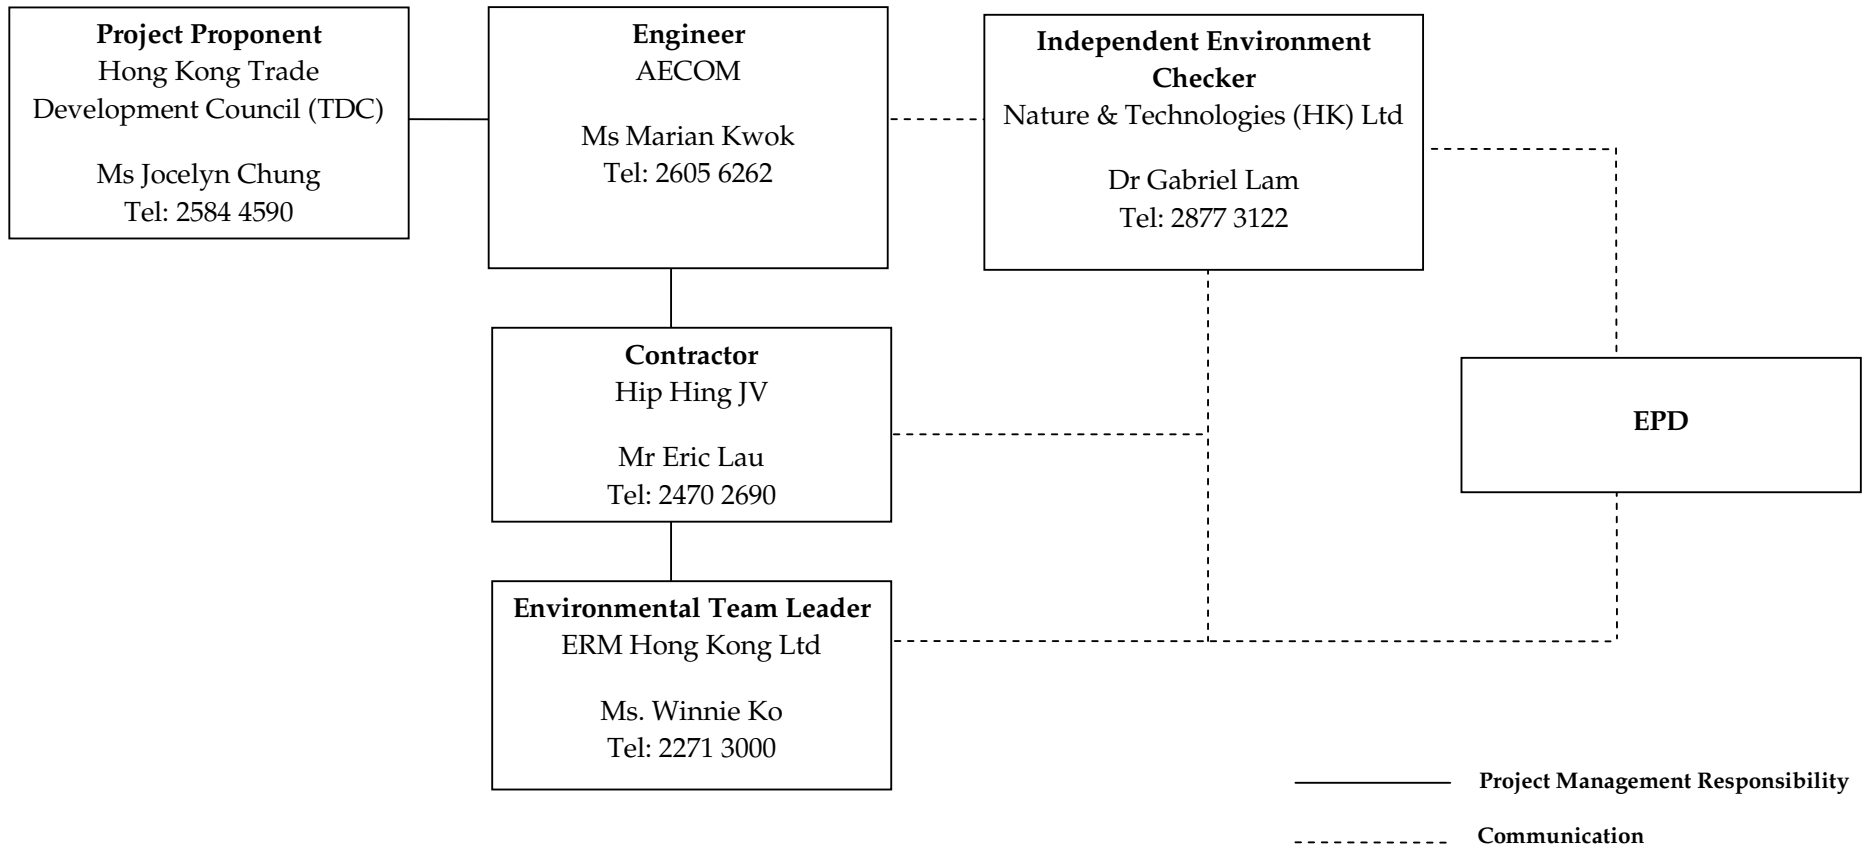

Annex C

Location of NO₂ Monitoring Station

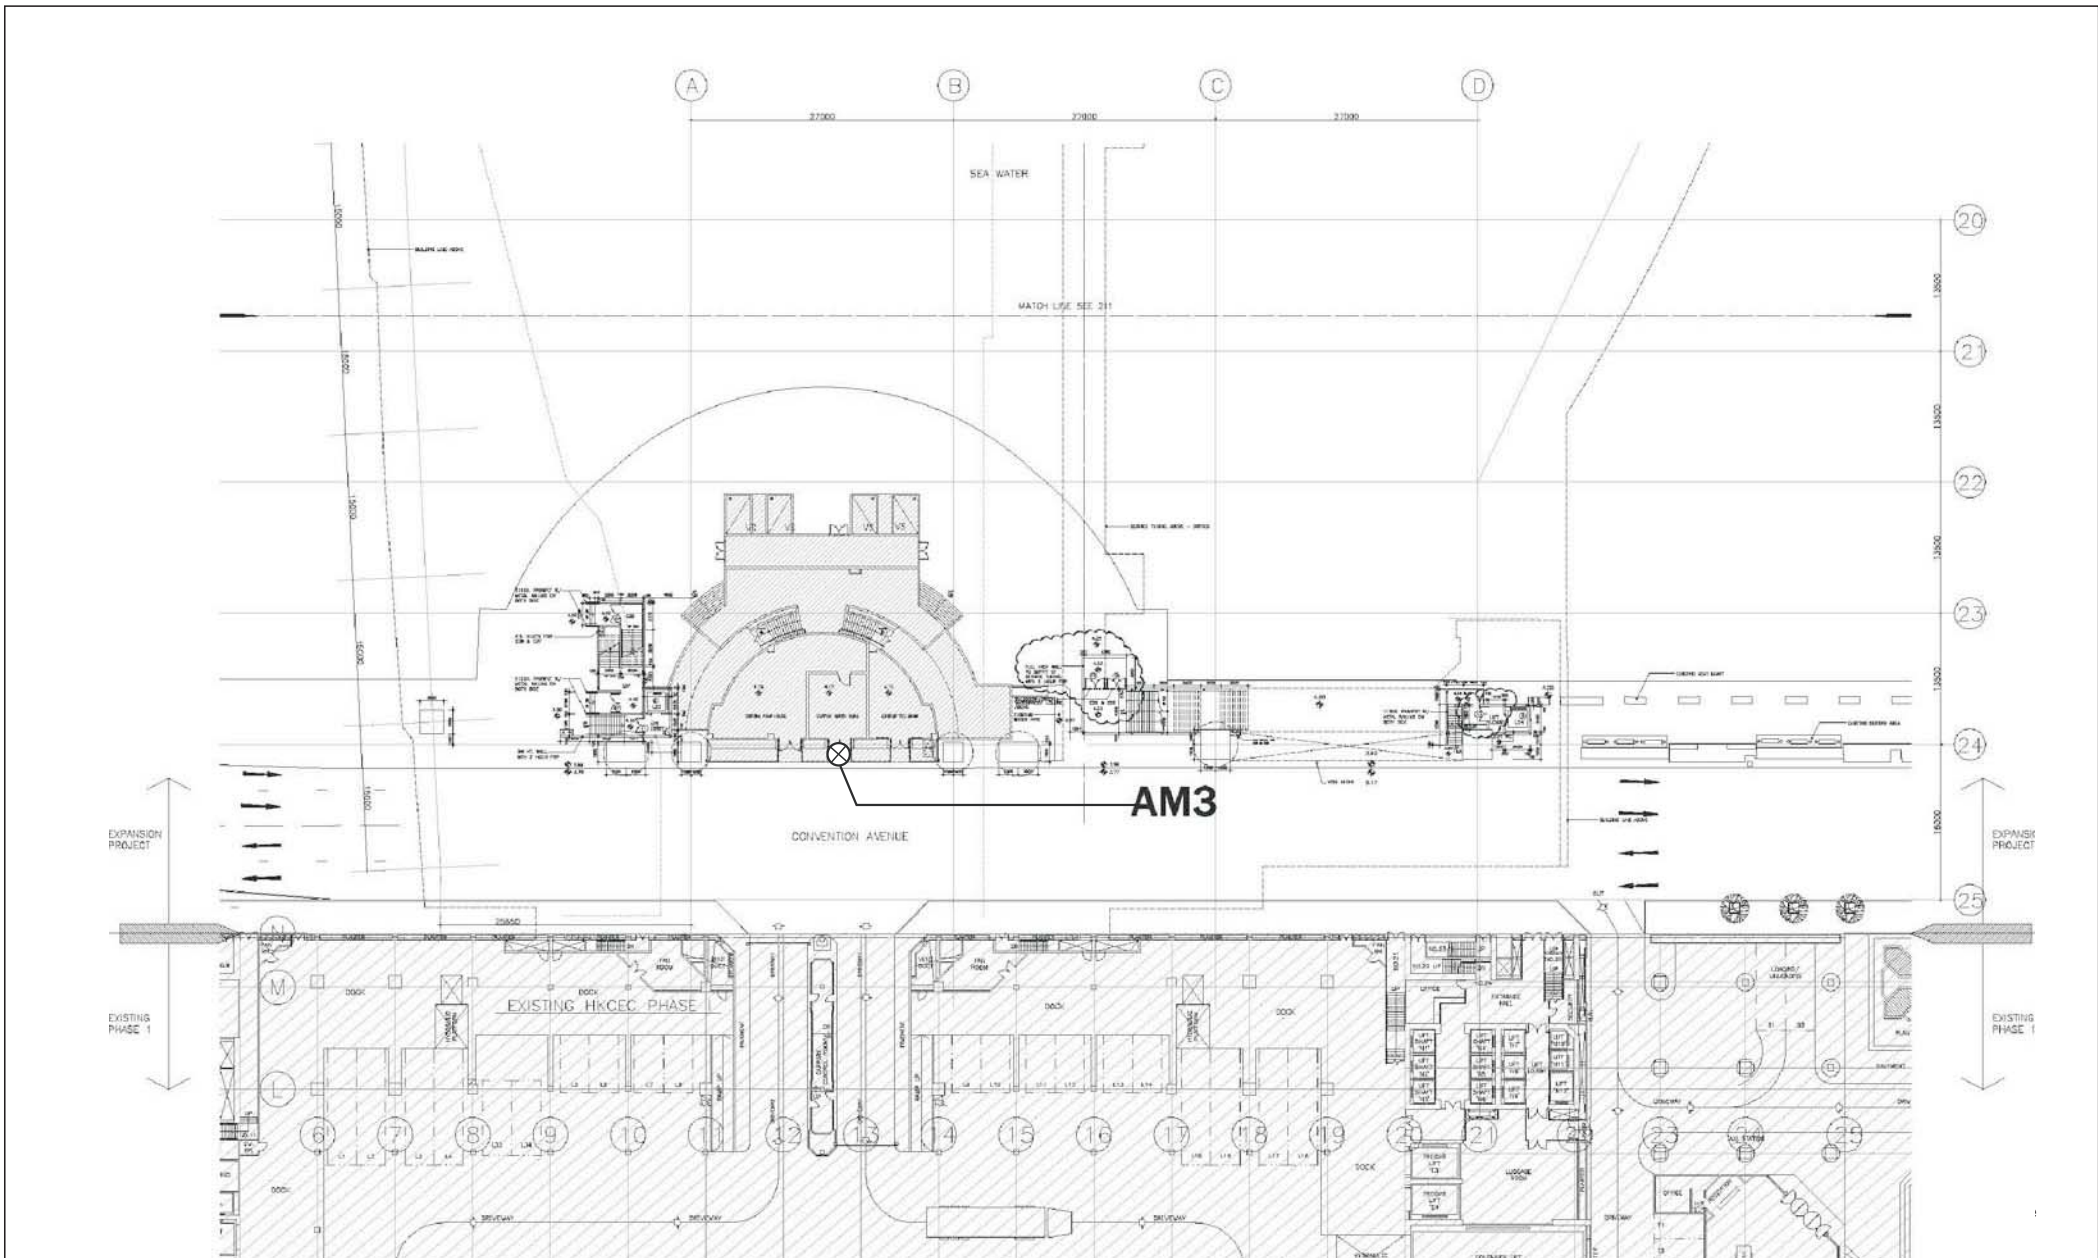


Figure C1

Location of NO₂ Monitoring Station

FILE: 0050690a
DATE: 06/08/2010

Environmental
Resources
Management



APPEARANCE OF NO₂ MONITORING STATION



NO₂ Monitoring Station (AM3)

Annex D

Monitoring Schedule for the Reporting Period and Next Month

**Hong Kong Convention and Exhibition Centre, Atrium Link Extension
Operational Phase Air Quality Monitoring Schedule - December 2010 and January 2011**

Sunday	Monday	Tuesday	Wednesday	Thursday	Friday	Saturday
			1-Dec	2-Dec	3-Dec	4-Dec
			24-hour monitoring	24-hour monitoring	24-hour monitoring Flow check	24-hour monitoring
5-Dec	6-Dec	7-Dec	8-Dec	9-Dec	10-Dec	11-Dec
24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	2-point calibration 24-hour monitoring Flow check Replace filter	24-hour monitoring
12-Dec	13-Dec	14-Dec	15-Dec	16-Dec	17-Dec	18-Dec
24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring Flow check	24-hour monitoring
19-Dec	20-Dec	21-Dec	22-Dec	23-Dec	24-Dec	25-Dec
24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring Replace filter Flow check	24-hour monitoring
26-Dec	27-Dec	28-Dec	29-Dec	30-Dec	31-Dec	1-Jan
24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring Flow check Multi-point calibration check	24-hour monitoring
2-Jan	3-Jan	4-Jan	5-Jan	6-Jan	7-Jan	8-Jan
24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	24-hour monitoring	2-point calibration 24-hour monitoring Flow check Replace filter	24-hour monitoring
9-Jan	10-Jan					
24-hour monitoring	24-hour monitoring					

Annex E

Calibration Certificates for
NO₂ Analyzer, Flow Meter
and Certificates for
Calibration Gas

TEST REPORT

APPLICANT: Cinotech Solution Limited
1710, Technology Park,
18 On Lai Street,
Shatin, N.T.
Cinotech Solution Limited

Test Report No.:	11603
Date of Issue:	2010-07-09
Date Received:	2010-07-06
Date Tested:	2010-07-08
Date Completed:	2010-07-08
Next Due Date:	2011-07-08

ATTN: Mr. William Lai

Page: 1 of 1

Certificate of Calibration

Item for calibration:

Description	: Flow meter
Manufacturer	: Bios International
Model No.	: DCL-M
Serial No.	: 109999

Test conditions:

Room Temperature	: 23 degree Celsius
Relative Humidity	: 56%

Test Specifications:

Performance checking of the flowrate around 100mL/min, 500mL/min and 800mL/min.

Methodology:

The flow meter is tested by comparing it to calibrated flowmeter (E348). High-purity nitrogen gas and flowcontroller are used as source of the gas flow. Records of the testing flowmeter and calibrated flowmeter are as following table.

Results:

E348	DCL-M	% Diff	Acceptable Criteria	Result
Instrument reading (mL/min)	Instrument reading (mL/min)			
114.5	114.7	0.17	+ 3%	Pass
521.3	519.4	-0.36	+ 3%	Pass
780.6	773.1	-0.96	+ 3%	Pass

PREPARED AND CHECKED BY:

For and On Behalf of **WELLAB Ltd.**


PATRICK TSE
Laboratory Manager

Calibration Certificate

General

Location:	Atrium Link
Calibration Date:	7-Jan-11
*Calibration Period:	15:15 - 15:50
Conducted by:	William Lai

* Including administration time

Equipment

Testing gas used:	Nitrogen Oxide, NO
Temperature:	~26 (°C)

Calibration Result

No.	Time Stamp	Type & Standard	Quantity (ppb)	Stability (ppm)	Result
1	7 January 2011 15:15	Pure (0 ppb) ± 15 ppb[1] =	-0.1245	0.0343	(PASS)
2	7 January 2011 15:50	NO (400 ppb) ± 15 %[1] =	398.4322	0.2124	(PASS)

*NO Slope [2]: 1.0923

* The NO Slope acceptable limit should be within 1.000 ± 0.300 .

Coordinated and Conducted By:


Staff in charge



Reference:

[1] Page2, 2.3.5, 2.3 QA & QC Procedure, Method Statement Report - NO2 Monitoring underneath Atrium Link Extension

[2] "NO SLOPE"Function, Table 10-6: Calibration Data Quality Evaluation, P.197, 10.6 Calibration Quality Analysis, M200E Nox Analyzer Technical Manual

Calibration Certificate

General

Location:	Atrium Link
Calibration Date:	10-Dec-10
*Calibration Period:	17:00 - 17:45
Conducted by:	William Lai

** Including administration time*

Equipment

Testing gas used:	Nitrogen Oxide, NO
Temperature:	-27 (°C)

Calibration Result

No.	Time Stamp	Type & Standard	Quantity (ppb)	Stability (ppm)	Result
1	10 December 2010 17:00	Pure (0 ppb) ± 15 ppb ^[1] =	-0.1245	0.0372	(PASS)
2	10 December 2010 17:45	NO (400 ppb) ± 15 % ^[1] =	403.0498	0.3415	(PASS)

*NO Slope [2]: 1.0532

** The NO Slope acceptable limit should be within 1.000 ± 0.300.*

Coordinated and Conducted By:

[Signature]


Staff in charge



Reference:

[1] Page2, 2.3.5, 2.3 QA & QC Procedure, Method Statement Report - NO2 Monitoring underneath Atrium Link Extension

[2] "NO SLOPE" Function, Table 10-6: Calibration Data Quality Evaluation, P.197, 10.6 Calibration Quality Analysis, M200E Nox Analyzer Technical Manual



HONG KONG SPECIALTY GASES CO., LTD.

HSG – A companion for excellence

CERTIFICATE OF ANALYSIS

PRODUCT

CONCENTRATION

HP Grade
NITROGEN

99.995%

O₂

< 10 ppm

H₂O

< 10 ppm

Authorized Signature

2/F, Blk B, Wing Cheong Fty Bldg., No. 121 King Lam St., Cheung Sha Wan, Kln, HK

TEL: (852) 2668 5738

FAX: (852) 2652 0401

Website: <http://www.hsg.com.hk>






CERTIFICATE OF ANALYSIS

Customer Name:	Cinotech Consultants Ltd	Cylinder Number:	CC87834
Stock or Analyzer Tag Number:	N/A	Product Class:	Primary NIST Standard
Customer Reference:	PO-10008	Cylinder - Contents ¹ :	140 CF @ 2000 PSI
MESA Reference:	107693	Cylinder-CGA:	A030-HP-SS/660
Date of Certification:	6/22/2010	Analysis Method:	Process Analyzers
Recommended Shelf Life:	1 Year	Preparation Method:	Gravimetric

Component*	Requested Concentration ²	Reported Concentration ^{2,3}
Nitric Oxide	400ppb	400±20ppb
Nitrogen Dioxide		<2ppb
Nitrogen	Balance	Balance

*Ref to SRM 2627a

Authorized Signature: 

1. The fill pressure shown on the COA is as originally quoted. The fill pressure measured by the customer may differ from the fill pressure originally quoted due to temperature effects, compressibility of the individual components when blended together in the cylinder, gauge accuracy or reduction in content volume before shipping as a result of samples withdrawn for laboratory QC necessary to ensure product quality.
2. Unless otherwise stated, concentrations are given in molar units.
3. Vapor pressure mixes are blended at a sufficiently low pressure so as to eliminate phase separation under most low temperature conditions encountered during transport or storage. However, it is generally recommended that cylinders containing vapor pressure restricted mixes be placed on the floor in a horizontal position and rolled back and forth to improve homogeneity of the gas phase mixture before being put into service.

Analytical Gas Standards are prepared and analyzed using combinations of NIST traceable weights, SRM's provided by NIST, or internal gas standards that have been verified for accuracy using procedures published by the US-EPA. Pure gases are analyzed and certified for purity using minor component Analytical Gas Standards prepared according to the methods specified above. Balances are calibrated to NIST test weights covered by NIST test number 822/256175/96. Reference Certification #'s: 163/W, 830/N and 3280. Calibration methods are in conformance with MIL-STD 45662A.

MESA Specialty Gases & Equipment

division of MESA International Technologies, Inc.

2427 South Anne St ♦ Santa Ana, California 92704 ♦ USA

TEL: 714-434-7102 ♦ FAX: 714-434-8006 ♦ E-mail: mail@mesagas.com

On-line Catalog at www.mesagas.com

Cole Parmer Instrument Co.

Calibration Data Sheet

Certification Number: 0000049715

Sales Order Number: SO304015
Serial Number: 56090
Part Number: 32907-67
Software Version: GP07R93
P/D/I Values: 100 / 12000 / 0
Process Gas: Selectable
Calibration Gas: Air
Range: 1 SLPM
Gas Temperature: 24.9 °C
Ambient Humidity: 42%
Calibration Procedure/Rev. #: DOC-AUTOCAL-GASFLOW/Rev. 60
Calibrated By: Jamie Wilde
Calibration Date: 09/01/2010
Full Scale Pressure: 160 PSIA
Full Scale Pressure Accuracy: +/-0.5% of Full Scale
Temperature Accuracy: +/-1.5 °C
Standard Temp. & Pressure: 25°C, 14.6959 PSIA
Calibration due 1 yr. after receipt:

Equipment Used

Temperature: TOOL-TEMP6	Voltage: TOOL-CMTR12
Tool Due Date: 07/08/2011	Tool Due Date: 07/08/2011
Manufacturer/Model: ERTCO	Manufacturer/Model: Fluke 85
NIST #: 33173	NIST #: 664133-7971257:1272460434
Device Uncertainty: +/- 0.2 deg C	Device Uncertainty: +/- (0.1% + 1 digit)
Flow: TOOL-FLOW4	Pressure: TOOL-PRESSURE8
Tool Due Date: 05/10/2011	Tool Due Date: 04/23/2011
Manufacturer/Model: Alicat / MCAL-1E0L	Manufacturer/Model: Alicat / P-100PSIG-D
NIST #: 62225-68342	NIST #: 936034-76650613:1143713248
Device Uncertainty: +/- (0.3% Reading + 0.2% F.S.)	Device Uncertainty: +/- 0.2%

All test equipment used for calibration is NIST traceable.

Calibration

Uncertainty: +/- (0.8% of Reading + 0.2% of Full Scale)
Units of measure: SLPM

Calibration Pressure: Inlet: 10 PSIG
Outlet: 0 PSIG

Output 1 Configuration Output 2 Configuration
Mini-Din Pin #6 Mini-Din Pin #2

D.U.T.	Actual	In Tolerance	Output 1	Output 2
0.000	0.000	Yes	0.000 Vdc	5.12 Vdc
0.250	0.250	Yes	1.250 Vdc	5.12 Vdc
0.499	0.500	Yes	2.495 Vdc	5.12 Vdc
0.747	0.750	Yes	3.735 Vdc	5.12 Vdc
0.999	0.999	Yes	5.00 Vdc	5.12 Vdc

Notes: 0-5V set-point.

Tech Signature: 

QC Signature: 

Calibration performed by Alicat Scientific, Inc.

CS1 Rev 14 Last Modified 04/17/2007

Cole Parmer Instrument Co.

Calibration Data Sheet

Certification Number: 0000049714

Sales Order Number: SQ304015
Serial Number: 56089
Part Number: 32907-67
Software Version: GP07R93
P/D/I Values: 100 / 12000 / 0
Process Gas: Selectable
Calibration Gas: Air
Range: 1 SLPM
Gas Temperature: 24.9 °C
Ambient Humidity: 42%
Calibration Procedure/Rev. #: DOC-AUTOCAL-GASFLOW/Rev. 60
Calibrated By: Jamie Wilde
Calibration Date: 09/01/2010
Full Scale Pressure: 160 PSIA
Full Scale Pressure Accuracy: +/- 0.5% of Full Scale
Temperature Accuracy: +/- 1.5 °C
Standard Temp. & Pressure: 25°C, 14.6959 PSIA
Calibration due 1 yr. after receipt:

Equipment Used

Temperature: TOOL-TEMP6
Tool Due Date: 07/08/2011
Manufacturer/Model: ERTCO
NIST #: 33173
Device Uncertainty: +/- 0.2 deg C

Flow: TOOL-FLOW4
Tool Due Date: 05/10/2011
Manufacturer/Model: Alicat / MCAL-1E0L
NIST #: 62225-68342
Device Uncertainty: +/- (0.3% Reading + 0.2% F.S.)

Voltage: TOOL-CMTR12
Tool Due Date: 07/08/2011
Manufacturer/Model: Fluke 85
NIST #: 664133-7971257.1272460434
Device Uncertainty: +/- (0.1% + 1 digit)

Pressure: TOOL-PRESSURE8
Tool Due Date: 04/23/2011
Manufacturer/Model: Alicat / P-100PSIG-D
NIST #: 936034-76650613:1143713248
Device Uncertainty: +/- 0.2%

All test equipment used for calibration is NIST traceable.

Calibration

Uncertainty: +/- (0.8% of Reading + 0.2% of Full Scale)
Units of measure: SLPM


Calibration Pressure: Inlet: 10 PSIG
Outlet: 0 PSIG

Output 1 Configuration Output 2 Configuration
Mini-Din Pin #6 Mini-Din Pin #2

D.U.T.	Actual	In Tolerance	Output 1	Output 2
0.000	0.000	Yes	0.000 Vdc	5.12 Vdc
0.249	0.250	Yes	1.245 Vdc	5.12 Vdc
0.499	0.500	Yes	2.495 Vdc	5.12 Vdc
0.748	0.750	Yes	3.740 Vdc	5.12 Vdc
0.999	1.000	Yes	5.000 Vdc	5.12 Vdc

Notes: 0-5V set-point.

Tech Signature: _____

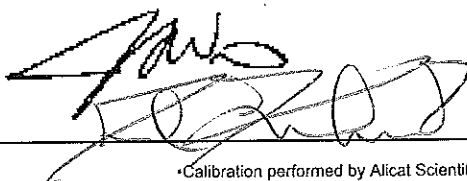

QC Signature: _____

• Calibration performed by Alicat Scientific, Inc. •

CS1 Rev 14 Last Modified 04/17/2007

Annex F

Event Action Plans for Air Quality Monitoring

Table F1 Event Action Plans for Air Quality

Event	Action	
Action Level being exceeded in the monitoring station	ET	TDC
	<ul style="list-style-type: none"> • Notify TDC; • Provide details of AQO exceedance and monitoring condition to EPD; 	<ul style="list-style-type: none"> • Liaise with EPD to investigate mitigation proposals; • Implement mitigation proposals, if required.

Annex G

NO₂ Monitoring Results

Annex G - Summary of Hourly Average of NO₂ at AM3

Hourly Average NO ₂ (µg/m ³) in Reporting Month																
Time / Date	1-Dec-10	2-Dec-10	3-Dec-10	4-Dec-10	5-Dec-10	6-Dec-10	7-Dec-10	8-Dec-10	9-Dec-10	10-Dec-10	11-Dec-10	12-Dec-10	13-Dec-10	14-Dec-10	15-Dec-10	
0:00	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	
1:00	60.8	69.6	47.6	35.7	63.5	138.7	42.1	58.1	92.0	46.3	51.8	46.2	45.9	67.7	37.9	
2:00	62.2	50.4	38.5	34.7	49.2	146.4	24.9	51.4	99.7	41.9	43.2	38.2	35.5	54.7	24.3	
3:00	73.8	52.3	39.0	26.8	34.3	142.4	21.7	37.8	104.0	32.1	30.4	26.3	34.3	99.7	22.8	
4:00	49.6	31.1	53.0	21.7	33.8	130.2	22.2	30.9	93.1	22.2	37.8	27.0	27.3	51.7	21.5	
5:00	40.9	30.1	37.8	21.7	32.3	119.9	27.0	27.9	96.0	28.7	42.2	41.2	26.9	55.9	21.1	
6:00	57.0	54.3	64.2	41.8	45.4	124.6	35.6	54.6	63.3	41.4	40.3	37.3	40.1	54.3	29.6	
7:00	93.3	89.5	95.5	54.2	81.5	171.0	68.0	89.2	107.3	68.2	66.2	43.6	70.9	64.8	46.2	
8:00	151.2	163.3	162.5	78.7	86.1	207.8	130.7	129.3	154.8	131.2	99.7	50.7	120.2	124.7	88.2	
9:00	162.3	175.8	152.9	101.3	90.8	239.9	134.2	151.0	193.9	148.5	125.0	62.5	143.0	191.5	109.4	
10:00	123.9	155.4	100.4	116.1	117.9	202.6	117.7	135.4	116.8	122.6	104.8	63.0	105.3	117.5	158.0	
11:00	134.8	146.3	77.0	106.9	113.9	152.7	111.2	133.4	106.4	125.6	119.0	82.7	99.7	99.7	80.9	
12:00	135.3	172.3	117.7	158.3	128.8	170.8	119.2	148.2	92.6	118.0	108.9	72.3	121.5	114.8	74.8	
13:00	117.4	178.3	131.6	168.6	120.5	131.5	127.3	161.7	99.0	95.2	107.0	71.5	142.6	113.0	69.4	
14:00	138.4	201.5	120.9	140.5	110.9	116.4	129.6	130.3	96.6	104.2	101.6	81.2	112.2	101.8	91.3	
15:00	128.7	259.9	151.2	149.8	135.7	170.8	140.2	138.9	128.9	118.1	95.6	70.8	145.5	132.5	94.1	
16:00	141.6	293.2	87.9	172.1	171.0	152.8	152.6	138.1	148.5	99.6	97.0	82.8	150.2	128.8	97.7	
17:00	146.6	283.9	157.4	161.9	175.3	193.1	162.4	151.5	181.1	99.6	168.5	87.5	162.6	112.9	107.8	
18:00	214.6	241.8	144.0	218.6	163.4	179.3	161.0	152.9	191.3	161.9	129.7	101.9	141.5	81.0	105.1	
19:00	183.7	241.1	138.4	152.5	157.0	157.5	137.8	133.0	146.9	155.9	110.9	100.2	148.5	72.2	124.3	
20:00	166.9	165.4	87.5	144.7	160.9	131.6	122.1	136.1	159.8	106.7	101.1	107.9	115.1	64.2	132.5	
21:00	131.2	136.9	59.8	103.0	153.1	141.8	104.6	115.3	115.0	74.4	81.0	86.5	90.8	62.7	57.4	
22:00	96.1	81.6	58.2	107.3	153.4	105.1	101.5	107.8	95.1	86.9	69.9	78.5	80.8	55.6	46.5	
23:00	101.7	68.5	56.6	89.6	170.3	79.6	93.3	91.4	79.3	98.6	59.0	79.4	89.2	62.3	44.0	


Remarks
 - Analyzer Calibration in Progress
 z/s Zero-span check in progress. Less than 40 minutes of data is collected in the reporting period and is therefore not presented.
 * Less than 40 minutes of valid data is collected in the period and is therefore flagged and not presented
 - Multi-point calibration check in progress

Hourly Average NO ₂ (µg/m ³) in Reporting Month																
Time / Date	16-Dec-10	17-Dec-10	18-Dec-10	19-Dec-10	20-Dec-10	21-Dec-10	22-Dec-10	23-Dec-10	24-Dec-10	25-Dec-10	26-Dec-10	27-Dec-10	28-Dec-10	29-Dec-10	30-Dec-10	31-Dec-10
0:00	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s
1:00	36.0	38.5	141.5	80.4	187.0	132.0	184.1	69.3	54.3	35.1	36.0	84.5	130.5	160.1	73.8	47.7
2:00	30.4	27.9	111.7	50.1	174.0	128.4	172.9	40.1	72.6	32.3	34.6	66.2	86.1	135.8	105.2	44.6
3:00	29.7	36.4	105.8	45.7	116.2	162.4	35.7	54.5	27.4	28.6	57.8	88.1	120.0	65.1	47.8	50.8
4:00	24.1	34.4	113.7	56.4	154.5	102.0	134.4	33.4	32.8	21.1	32.3	88.5	122.0	125.0	67.8	50.8
5:00	21.3	42.0	102.0	47.7	143.9	106.0	119.6	30.8	42.8	20.9	24.2	115.2	112.7	106.2	96.2	41.4
6:00	26.8	48.8	66.0	55.5	145.6	108.8	106.1	45.1	48.8	24.6	27.7	105.1	126.7	91.1	110.1	56.9
7:00	48.6	79.4	76.4	66.4	134.4	131.0	106.6	99.0	64.1	27.8	42.6	106.8	161.2	137.9	133.6	109.4
8:00	83.3	122.7	111.2	85.5	208.1	164.9	140.1	196.9	102.5	39.6	61.0	100.3	208.1	192.6	139.5	159.8
9:00	86.7	157.5	96.6	80.5	229.1	256.0	165.5	144.4	121.0	50.4	68.4	97.2	228.5	145.3	164.9	226.0
10:00	68.2	161.8	93.1	87.9	154.3	299.9	125.4	113.4	105.2	47.1	74.2	91.3	161.8	89.8	113.8	145.0
11:00	77.9	175.2	83.8	77.0	120.7	172.9	109.4	125.7	77.6	54.8	74.0	77.6	139.4	109.8	123.9	170.5
12:00	77.2	164.2	112.0	87.7	114.6	173.3	104.7	140.6	122.8	61.0	84.2	73.5	129.4	77.0	130.0	131.8
13:00	82.8	130.4	144.4	94.9	115.8	209.0	135.6	145.9	119.5	59.9	70.6	92.6	135.0	80.9	161.4	105.5
14:00	91.6	157.9	130.2	104.3	117.7	240.6	106.7	139.2	103.3	72.0	87.9	95.3	136.0	84.6	129.1	98.8
15:00	122.3	254.4	163.6	97.0	155.8	197.8	119.7	172.6	136.2	79.0	93.8	121.6	199.2	105.9	139.2	95.3
16:00	80.7	162.3	167.8	106.0	158.8	203.2	192.0	160.4	156.3	89.8	87.3	122.3	169.9	132.2	197.3	-
17:00	102.6	239.5	136.7	150.3	153.7	214.3	129.2	215.8	160.5	65.1	99.2	99.9	123.3	157.6	151.8	-
18:00	129.0	270.4	123.6	196.3	192.4	172.6	164.2	175.1	115.9	75.3	100.2	144.3	167.6	161.5	145.0	-
19:00	103.9	265.2	141.1	248.3	152.8	195.6	130.0	161.3	89.1	64.3	109.0	172.2	190.3	159.0	137.6	-
20:00	104.9	161.5	129.6	225.5	140.2	162.1	123.5	161.0	98.1	62.1	106.4	171.6	164.1	130.5	117.3	126.1
21:00	78.0	135.6	104.0	225.1	150.3	137.5	107.9	127.8	62.4	62.8	84.9	133.6	152.8	108.7	103.9	115.1
22:00	77.7	116.2	99.9	224.3	151.9	163.4	94.7	106.6	61.0	60.7	74.2	162.7	165.2	109.9	91.3	106.3
23:00	78.5	134.9	97.5	216.1	176.3	173.9	119.7	95.0	62.5	47.5	54.8	169.2	156.9	107.7	80.2	115.1

Remarks
 - Analyzer Calibration in Progress
 z/s Zero-span check in progress. Less than 40 minutes of data is collected in the reporting period and is therefore not presented.
 * Less than 40 minutes of valid data is collected in the period and is therefore flagged and not presented
 - Multi-point calibration check in progress

Hourly Average NO ₂ (µg/m ³) in Reporting Month										
Time / Date	1-Jan-11	2-Jan-11	3-Jan-11	4-Jan-11	5-Jan-11	6-Jan-11	7-Jan-11	8-Jan-11	9-Jan-11	10-Jan-11
0:00	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s	z/s
1:00	96.2	29.9	41.2	32.6	40.1	65.8	50.4	73.9	119.8	50.1
2:00	44.6	24.1	37.8	28.9	32.0	61.6	43.6	73.3	114.5	35.0
3:00	41.2	20.2	30.8	27.3	29.6	54.4	37.5	63.2	105.6	31.4
4:00	31.6	17.6	39.5	26.7	29.0	51.3	34.1	60.6	78.0	33.6
5:00	32.6	18.2	33.5	30.9	25.8	45.0	33.9	61.8	84.5	37.9
6:00	33.3	21.5	49.2	36.1	32.1	39.3	45.4	58.6	67.3	46.2
7:00	54.7	36.0	78.5	55.9	65.9	47.2	63.3	60.9	58.8	81.1
8:00	59.9	42.8	128.0	89.7	97.3	72.6	108.6	88.1	99.0	119.8
9:00	59.7	53.3	135.4	124.6	158.1	111.8	130.8	92.5	115.6	184.7
10:00	57.9	55.7	113.3	69.4	74.5	107.0	120.7	83.2	119.4	152.2
11:00	59.7	56.4	118.4	71.8	86.1	97.6	124.3	85.0	130.2	127.8
12:00	64.4	68.4	105.6	78.3	90.2	82.4	94.3	100.9	98.4	117.5
13:00	72.4	67.6	113.8	81.9	91.6	103.0	128.8	142.3	139.5	171.7
14:00	62.9	64.2	118.6	96.6	107.4	108.7	-	155.1	162.4	157.0
15:00	68.0	65.2	127.1	108.0	116.9	111.3	-	155.2	132.3	186.7
16:00	74.3	61.0	135.5	108.4	134.6	150.4	133.4	206.9	163.4	239.0
17:00	95.3	63.7	131.2	102.1	146.4	127.6	144.4	175.8	127.4	236.6
18:00	103.5	80.3	134.8	92.8	165.6	97.8	130.6	170.3	105.6	202.2
19:00	98.4	73.6	105.5	117.6	153.8	103.1	129.0	228.4	99.9	176.6
20:00	93.4	69.5	102.6	78.8	152.4	98.8	154.7	178.1	95.2	139.0
21:00	40.6	40.6	77.3	77.6	108.5	68.6	94.9	178.5	80.0	122.0
22:00	31.4	54.3	65.3							



Annex G - Graphical Presentation of Hourly Average of NO₂ at AM3

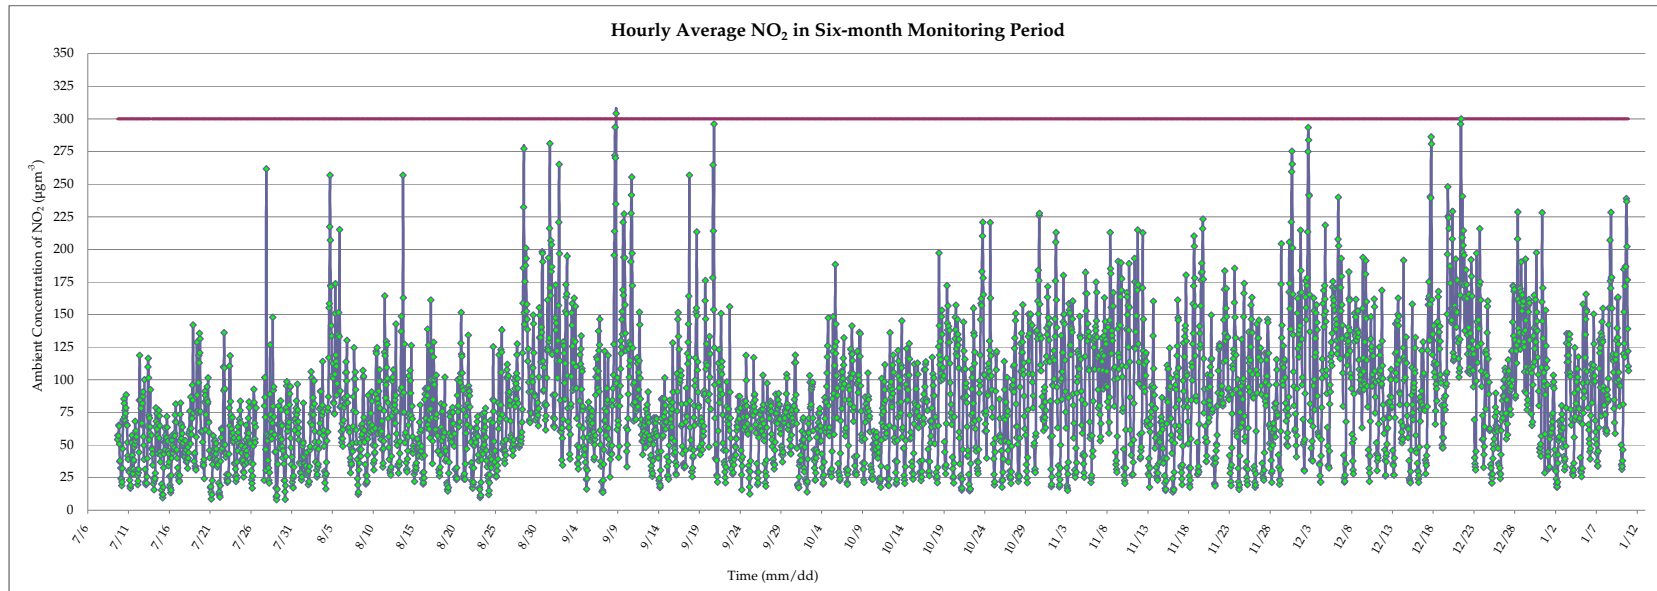

Remarks:

Automated zero-Span checks are conducted for approximately 30min from 0005 - 0035 hours daily. Less than 40 minutes of monitoring data is collected and thus a zero reading is presented at 12am daily.

Annex G - Graphical Presentation of Daily Zero-Span Check Results

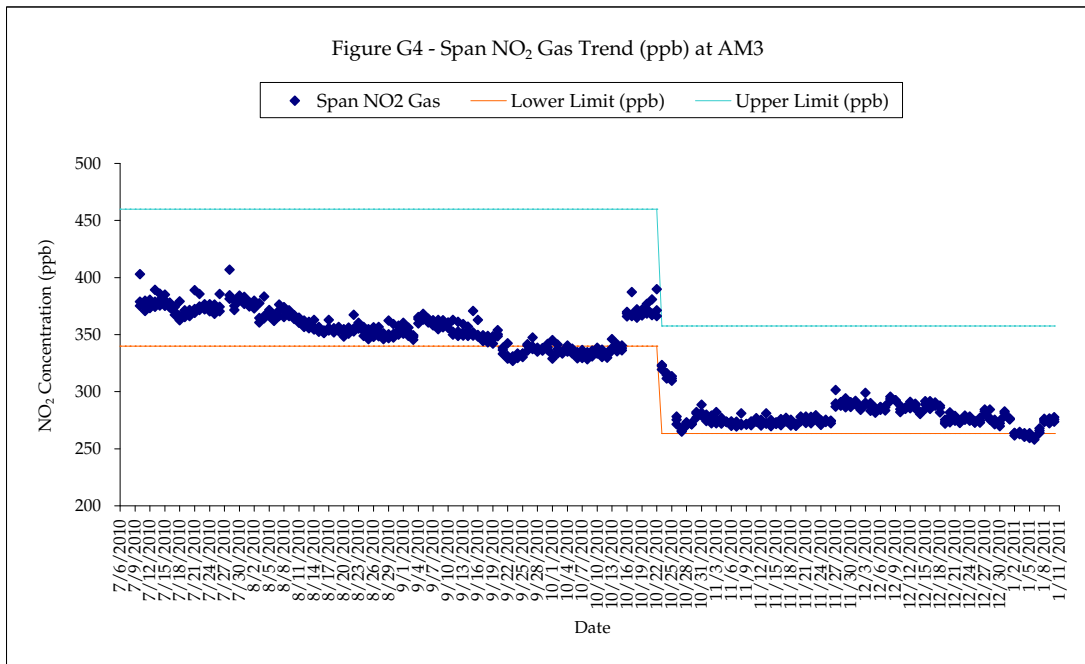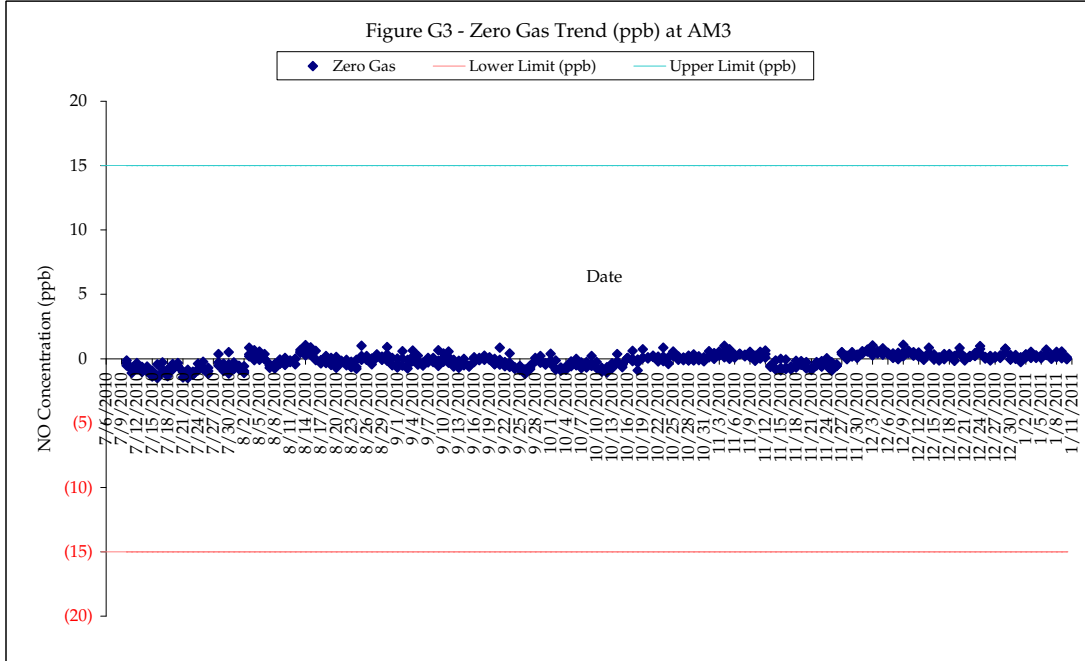

Annex G - Weekly Flowcheck Summary

NO₂ Analyzer Weekly Flowcheck

Sampling Flowcheck Results at AM3 (Under Atrium Link Extension)

Date	Avg. flow (cm ³ /min)	Avg. flow (cm ³ /s)	Required Flowrate by Specification of Equipment (cm ³ /s)	Compliance of Upper Flowrate Requirement (9.1 cm ³ /s)	Compliance of Upper Flowrate Requirement (7.5 cm ³ /s)
3-Dec-10	472.2	7.9	8.3±0.8	Y	Y
10-Dec-10	472.3	7.9	8.3±0.8	Y	Y
17-Dec-10	477.4	8.0	8.3±0.8	Y	Y
24-Dec-10	467.7	7.8	8.3±0.8	Y	Y
31-Dec-10	471.2	7.9	8.3±0.8	Y	Y
7-Jan-11	477.7	8.0	8.3±0.8	Y	Y

Annex G - Weekly Flowcheck Summary

NO₂ Analyzer Multi-point Calibration Check Results

Multi-point Check Results at AM3 (Under Atrium Link Extension) (performed on 31 December 2010)

Standard NO Gas Concentration by Mass Flow Controller (ppb)	Flow of Mass Flow Controller from 0ppb NO Gas (cm ³ /min)	Flow of Mass Flow Controller from 400ppb NO Gas (cm ³ /min)	NO Gas Concentration by Analyzer (ppb)	Necessary Adjustment of Measured Concentration
0	0.51	0.00	-0.11	0.11*
80	0.408	0.102	70.1	14.1%
149.8	0.319	0.191	147.7	1.4%
200	0.255	0.255	200.6	-0.3%
320	0.102	0.408	320.4	-0.1%
400	0.000	0.510	387.3	3.3%

Notes:

* - Drifting is absolute value